

Boston Brace Baby Order Form Instructions

Boston Baby Brace Order Form

Date: _____ Due Date: _____ PO #: _____ Contact: _____
 Ship To: _____ Ship Via: _____ Email: _____
 Address: _____ Account #: _____ Phone: _____
 City: _____ State: _____ Zip: _____ Previous Boston Baby Wearer Scan Label: _____

Patient Name: _____ HR: _____ in WT: _____ lbs
 Age: _____ Sex: _____ Diagnosis: _____

Anatomical Measurements All measurements required **Shape Capture**
 Scan Cast

	Cir.	M/L	A/P
Sternal Notch			
Axilla			
Xyphoid			
Waist			
Trochanter			

ASIS Anterior lateral relief

Brace Design

Liner
 3/16" Alplast Plastic 1/8" Copoly Other: _____
 Other: _____

Straps
 White Black

Pads
 .5" Installed .5" Un-Installed Unfinished Pads

1/8" Alplast Abdominal Cover

Transfer
 1st _____
 2nd _____

Boston Sensor
 Send Sensor
 Sensor Hole

CAD Design Section (DPSB Staff Only)

Lumbar/TL
 Left Right

TL Extension
 Height _____ cm

Thoracic Extension
 Left Right
 Height _____ cm

Axillary Extension
 Left Right

LAB USE ONLY

CAD OVEN DESIGN

FINISH PADS QC

Finished Heights *from waist

Sternal Notch: _____ cm Spine of Scap: _____ cm
 Pubis: _____ cm Axilla: _____ cm
 Trochanter: _____ cm
(Standard trochanters are standard)

Scol Tees
 Single Double Qty: _____

Notes:

Model 1200 (2022) Rev. 0 Boston Brace International, Inc. Boston DPSB is a company that is part of the GP Specialty Bracing division. 37 Shuman Ave Stoughton MA 02072 - customerservice@bostonoandp.com

Reminder – this form is for the technicians and goes with the flow of fabrication. All items on this form need to be completed to ensure customer service and manufacturing are able to fabricate the desired orthosis.

PLEASE DO NOT use this as your clinical note.

This form is for the fabrication of the Boston Brace Baby orthosis. Use this form if your patient is three-year-old or younger and presents with an idiopathic or congenital curve.

All items in bold are required (measurements) and represent the recommended standard.

The use of a thermal sensor is standard of care for infantile and congenital scoliosis. Discuss this with the parents/caregiver.

Demographics:

Date: Due Date: PO #: Contact:
 Ship To: Ship Via: Email:
 Address: Account #: Phone:
 City: State: Zip: Previous Boston Baby Wearer Scan Label:

Customer service uses this section to initiate the fabrication process. All of the above is entered into our system. In the event we need to contact you, the treating orthotist, or if you have a question on the fabrication, having this information entered allows for easy retrieval.

Previous Wearer:

Previous Boston Baby Wearer

Let us know if the patient has worn a Boston Baby brace before. If so, our technicians will notify you if there is a design change.

Scan label:

Scan Label:

Scan label is required to make sure the correct scan is modified.

Captevia: File name is auto-populated. The file will include both scans if taking a bivalve scan.

Laser scanner: Patient’s first initial, last name; scan number; clinicians’ initials; the word scoli; date of scan

i.e. patient John Smith is seeing clinician Jane Doe on April 1, 2020 for his first brace.

Scan Label: jsmith#1jdscoli04012020

Bivalve scan: Follow the sequence above and add _ant and _post after the date

Anterior section: jsmith#1jdscoli04012020_ant

Posterior section: jsmith#1jdscoli04012020_post

Patient Name, , Height, Weight Age, Sex, and Diagnosis:

Patient Name: _____ Ht: _____ ft _____ in Wt: _____ lbs
Age: _____ Sex: _____ Diagnosis: _____

Make sure the patient’s name is legible.

We will keep a secondary record for you showing the patient’s age, sex, height, (in feet and inches) and weight (in pounds). This information may assist in justifying a new orthosis.

Diagnosis is needed to complete records. Infantile idiopathic scoliosis (idiopathic scoliosis that is first diagnosed at 3 years of age and younger), congenital scoliosis (scoliosis secondary to a boney abnormality) and neuromuscular scoliosis.

Radiographic:

**Required	Lumbar/TL	Thoracic
Convexity	<input type="checkbox"/> Left <input type="checkbox"/> Right	<input type="checkbox"/> Left <input type="checkbox"/> Right
Apical Vertebra		
Cobb Angle		
Scoliometer Reading		

Review the patents x-ray and complete the table above by identifying the side of the convexity, apical Lumbar/Thoracolumbar (TL) and Thoracic apex and Cobb value(s). For single curves, add NA to appropriate box.

Anatomical Measurements:


Anatomical Measurements

*All measurements required

	Cir.	M/L	A/P
Sternal Notch	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Axilla	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Xyphoid	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Waist	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
Trochanter	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

Shape Capture

Scan Cast

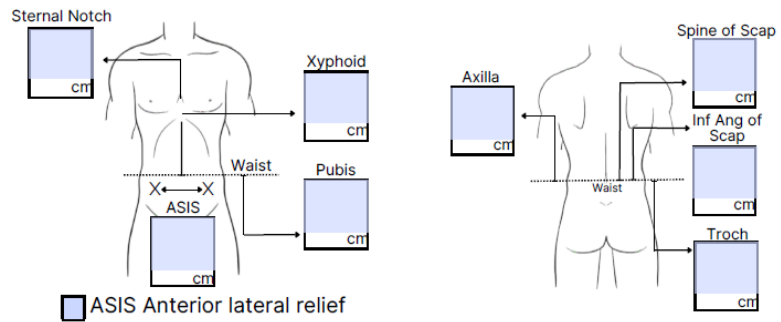

All Circumferential, ML AP, and linear measurements are required. All measurements are to be in centimeters. Note the distance from the waist to the greater trochanter. This will equate to the posterior inferior trim line.

Shape Capture

Indicate the method used to capture the patient's shape. This lets customer service know if they need to contact you or not if a scan is not attached to the order.

Shape Capture

Scan Cast

Brace Design

All Boston Brace Baby orthoses have a posterior opening to accommodate the anterior window.

Brace Design

Liner

3/16" Alipplast
 Other: _____

Plastic

1/8" Copoly
 Other: _____

Straps

White
 Black

Pads

.5" Installed
 .5" Un-Installed
 Unfinished Pads

1/8" Alipplast Abdominal Cover

Transfer

1st. _____
 2nd. _____

Liner, Plastic, and Straps:

Standard liner choice is 3/16” Aliplast. Standard plastic is 1/8” Copoly and standard straps are white. If a non-standard choice is desired, check the “Other” section and write the specific material in the other text box.

Pads:

Installed pads are the standard. Pads are pre-trimmed and skived per the curve pattern and brace design. Check the box to let us know how you want the pads to be provided.

1/8” Aliplast abdominal cover

An abdominal opening is standard with the Boston Baby. At times, this can cause a window edema and or discomfort

Transfer:

Choose their first and second choice of transfer using the Boston O&P transfer tool. (<https://www.bostonoandp.com/transfers/brace/>). Write the brace **transfer name** in this section. Every attempt will be made to provide the first choice.

Boston Sensor:

Boston Sensor
<input type="checkbox"/> Send Sensor
<input type="checkbox"/> Sensor Hole

The Boston Sensor adherence monitor is standard of care for the Boston Brace Baby orthoses. Sensors may be transferred to a patient’s subsequent brace.

Indicate if a Boston Sensor is to be sent with the brace.

If the patient has a sensor, and just needs to have the hole drilled into the brace, do not check the Send Sensor box, and only check the Sensor Hole box.

CAD Design:

CAD Design Section (OPSB Staff Only)

Lumbar/TL
 Left Right

TL Extension
Height _____ cm

Thoracic Extension
 Left Right
Height _____ cm

Axillary Extension
 Left Right

*Lower End Vertebra

The above section is optional.

If left blank, lab standards will be followed analyzing blueprinting the radiograph.

If you wish to design the brace, then this section needs to be COMPLETED in full. Partially completed work orders will require a call to the treating clinician and may delay fabrication.

The linear measurements represent both the dimensions of the internal pushes/shift as well as the orientation and position of the pads. These heights are based on the blueprint of the patient's x-ray and your clinical exam.

Lumbar/TL:


Indicate left or right lumbar/TL apex.

Lumbar/TL

Left Right

TL extension: is used for a TL apex or when L1/T12 vertebral bodies are deviated to the convex side of the caudal apex in a double curve. It will be to the side of the Lumbar/TL curve.

Push/Shift and Pad Dimensions:

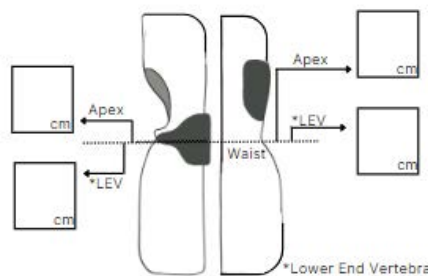

Indicate the dimension of the lumbar push and pad by writing in a whole number value for waist to apex and waist to lower end vertebra

Indicate the dimension of the thoracic push and pad by writing in a whole number value for waist to apex of the thoracic curve and waist to lower end vertebra.

Thoracic:

Indicate left or right thoracic apex. The height is to the midsagittal point of the thoracic extension.

Thoracic Extension

Left Right

Height cm

Axillary Extension:

Indicate left or right lumbar apex.

Axillary Extension

Left Right

To maximize the de-rotational effort of the Boston Brace Baby orthoses and to not impede breathing mechanics an open abdomen is standard. The kidney bean shape allows for this while providing a de-rotational force coupler.

The thoracic window maximizes the lateral shifting of the spine while also providing space for breathing.

The size and shape of both windows is determined by the shape of the patient and curve type. It is standard to cut out the abdominal window. It is standard to not cut out the thoracic window.

LAB USE ONLY

LAB USE ONLY		
CAD	OVEN	DESIGN
<input type="text"/>	<input type="text"/>	<input type="text"/>
FINISH	PADS	QC
<input type="text"/>	<input type="text"/>	<input type="text"/>

Our quality standards require each lab technician that completes a section of the fabrication process to identify themselves by writing their initials in the appropriate box.

Finish heights from waist:

Finished Heights <small>*from waist</small>	
Sternal Notch: <input type="text"/> cm	Spine of Scap: <input type="text"/> cm
Pubis: <input type="text"/> cm	Axilla: <input type="text"/> cm
	Trochanter: <input type="text"/> cm
(Bilateral trochs are standard)	

Finished heights measurements are used to finish the orthosis. All measurements use the waist as the base line.

Notes

Notes:



In the event a special request is made by the patient, or there is some unique anatomy or brace design needed that is not captured in the above sections, the notes section is where you may document this information.

Scoli T's:

Scoli Tees

White Single Double Qty:

If you are providing the patient with a Boston Scoliosis T shirt indicate the type and design (single or double axillary flap) along with the quantity. The size is determined from the submitted measurements.